



## FIG.2 SYRINGE ASSEMBLY






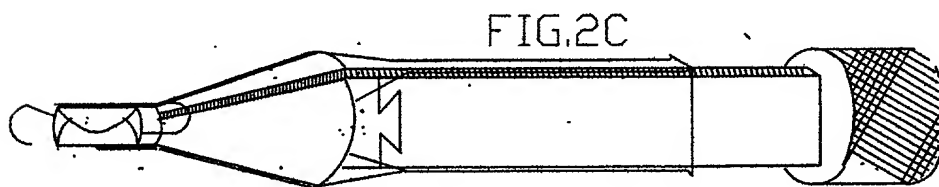



Fig 1A

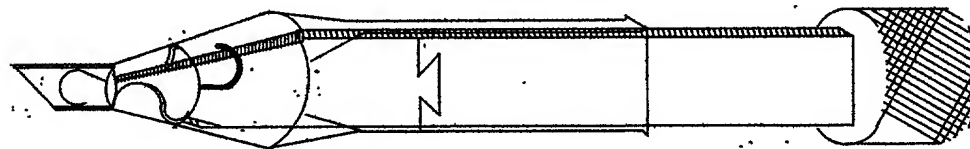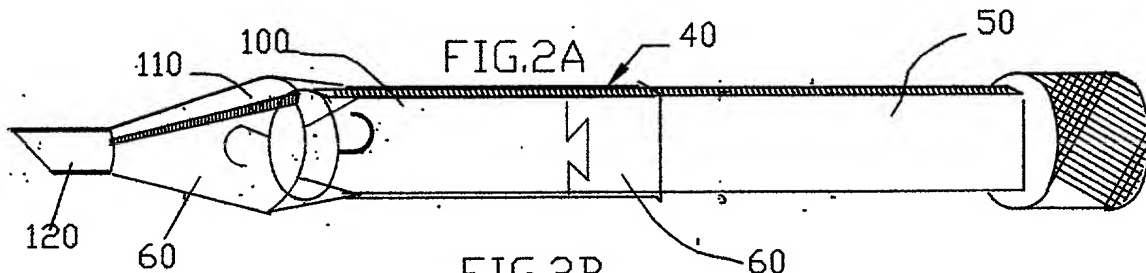
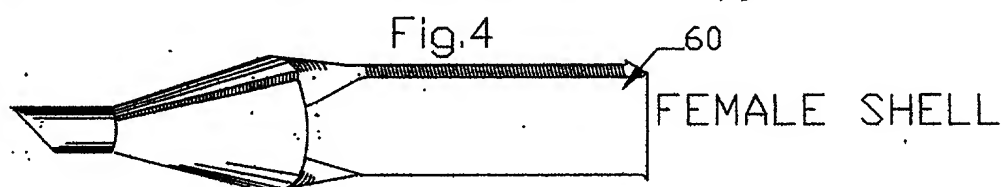


Furled Lens  
Enlarged

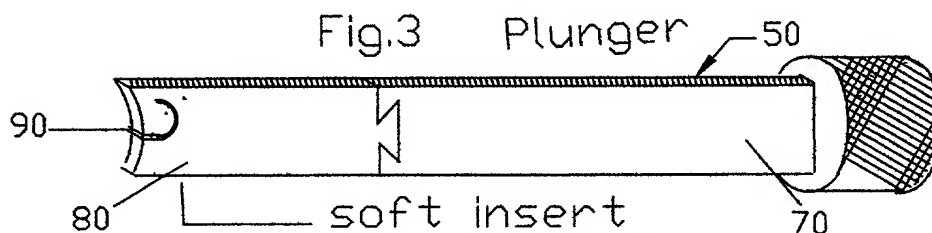

40

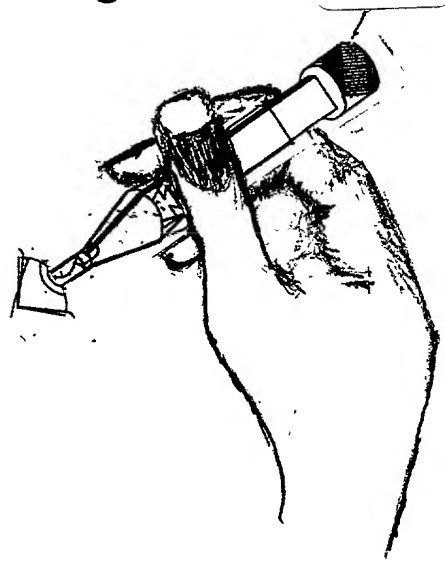[illegible]

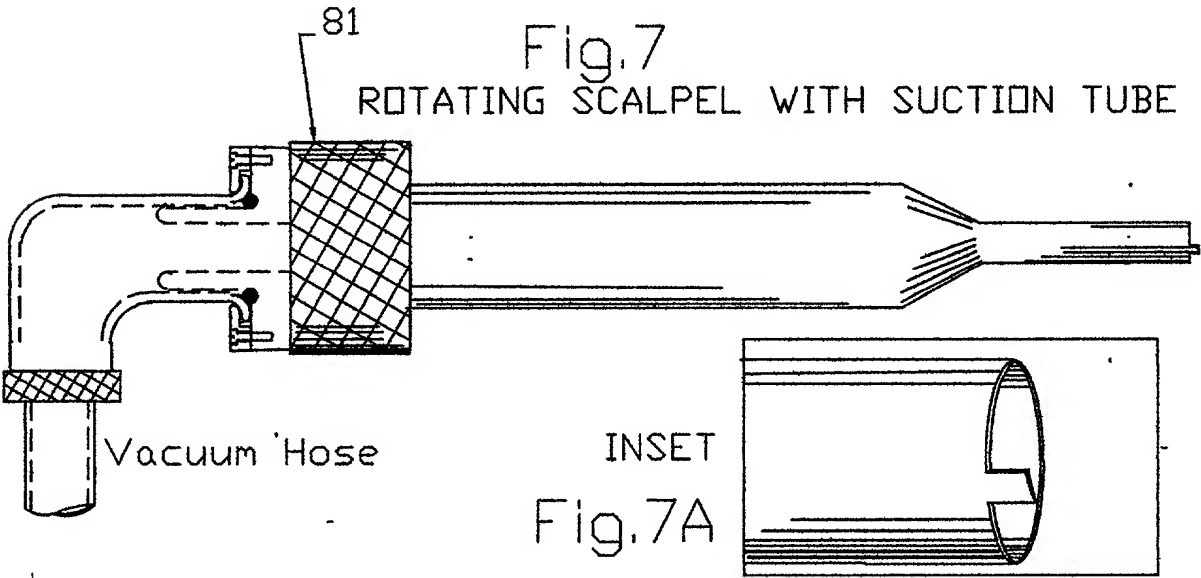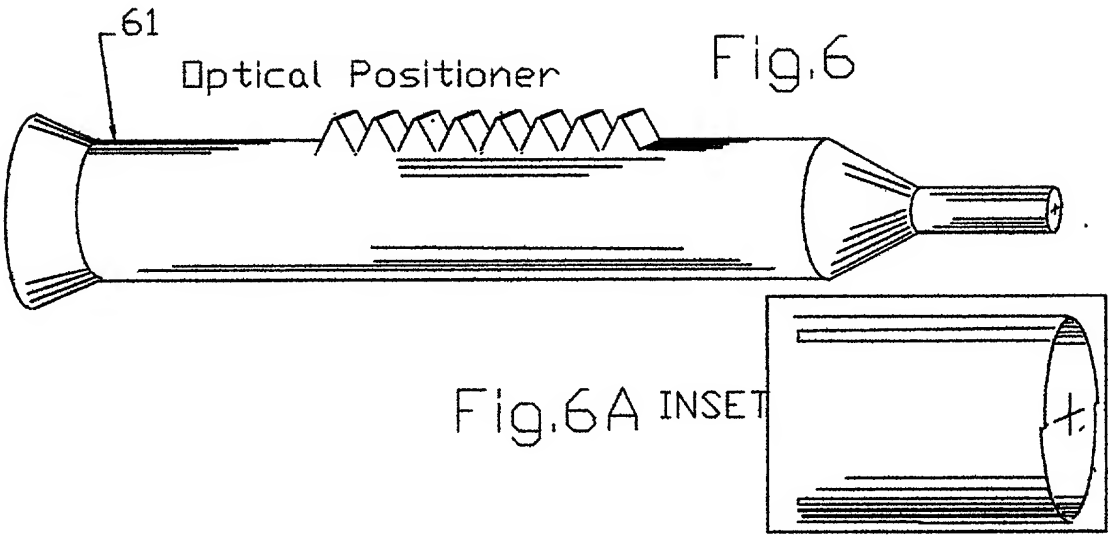

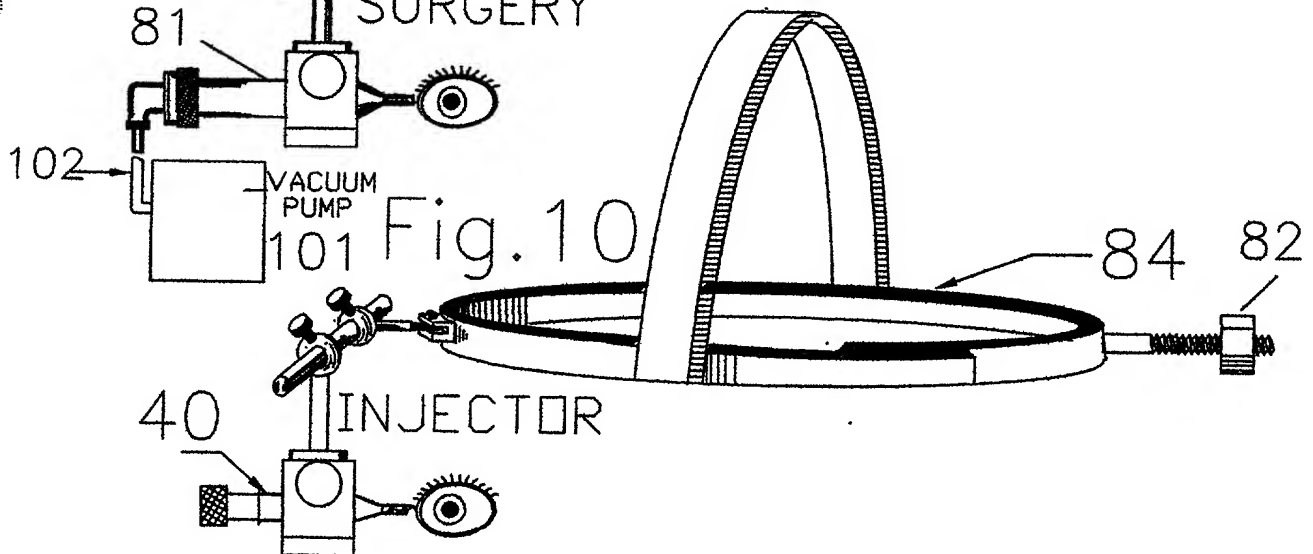
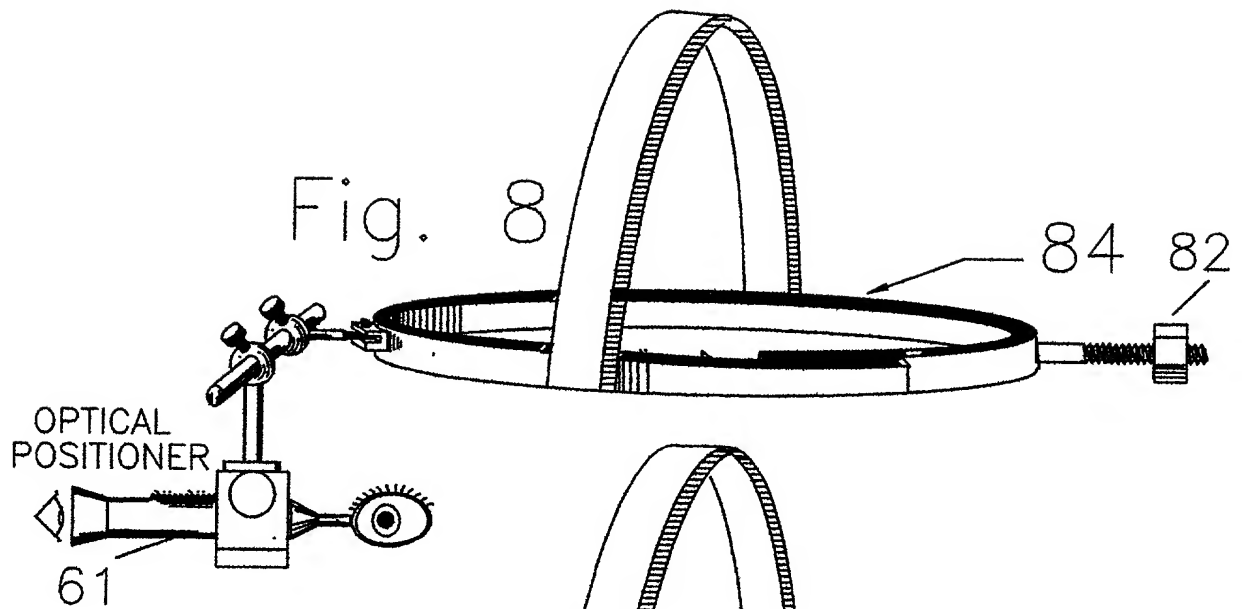


FIG.7 TURRET

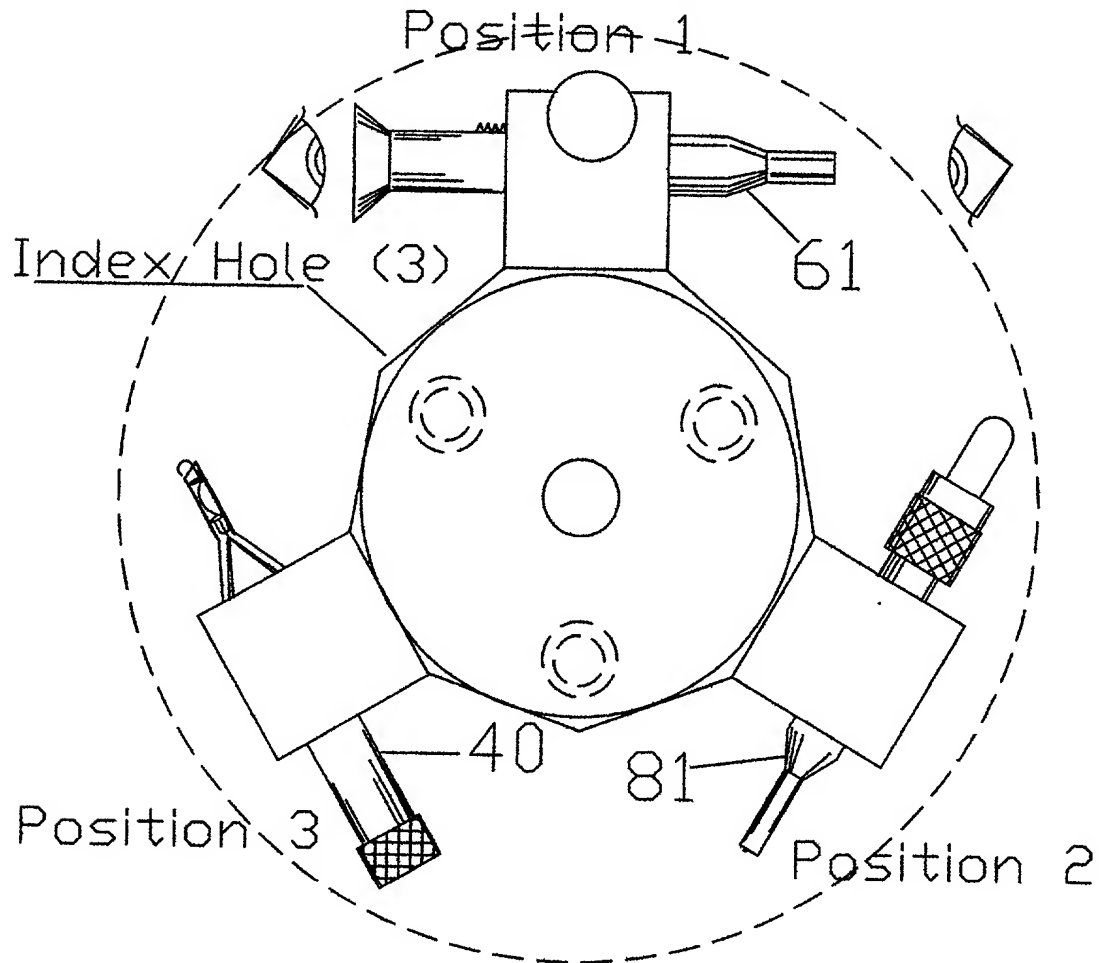


FIG. 7A

